

NANO ZS



Size Distribution Report by Volume

Sample Details

Sample Name: High_Tech_170622

SOP Name: NarrowHighRes.sop

General Notes: Average result created from record number(s): 73 74 75 76 77 78 79 80


File Name: CSL_2017.dts	Dispersant Name: Water
Record Number: 82	Dispersant RI: 1.330
Material RI: 1.25	Viscosity (cP): 0.8872
Material Absorbtion: 0.010	Measurement Date and Time: Thursday, June 22, 2017 12:...

System

Temperature (°C): 25.0	Duration Used (s): 90
Count Rate (kcps): 173.4	Measurement Position (mm): 4.65
Cell Description: Disposable sizing cuvette	Attenuator: 11

Results

	Diam. (nm)	% Volume	Width (nm)
Polydispersity Index: 0.403	Peak 1: 48.25	85.2	13.6
	Peak 2: 122.91	4.8	23.2
	Peak 3: 236.33	4.3	55.8

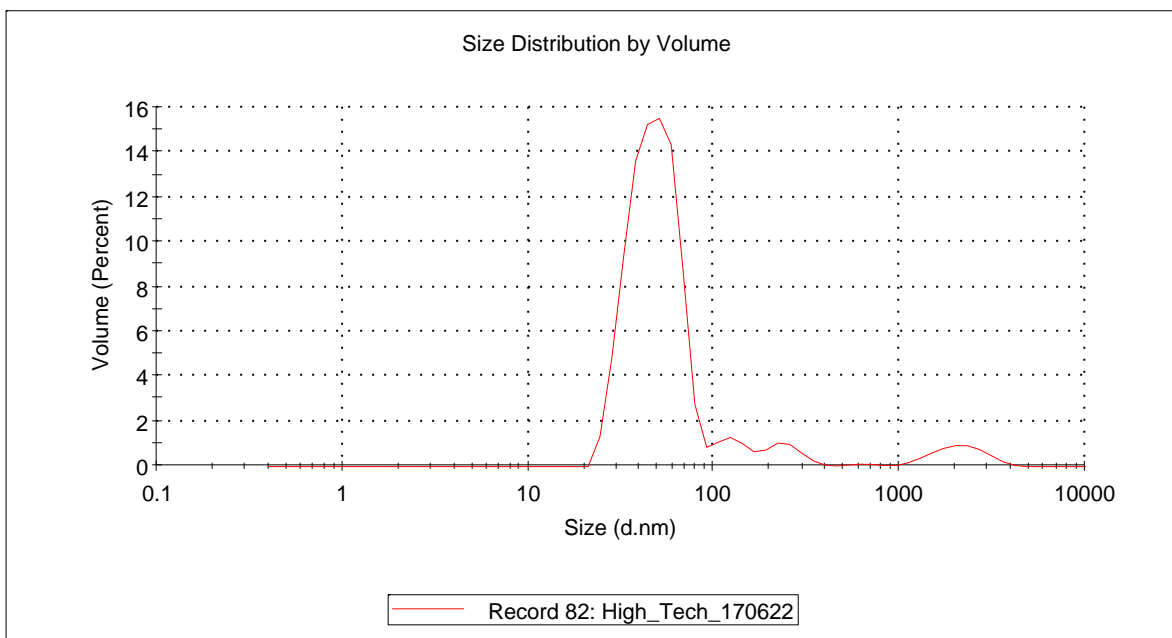

Colloidal Science Laboratory, Inc.

Westampton, NJ 609-267-2065